

Bioengineering 280A
Principles of Biomedical Imaging

Fall Quarter 2006
X-Rays Lecture 1

TT Liu, BE280A, UCSD Fall 2006

EM spectrum


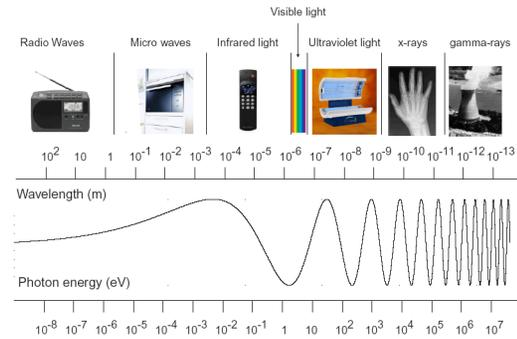


Figure 4.1: The electromagnetic spectrum.

TT Liu, BE280A, UCSD Fall 2006

Suetens 2002

X-Ray Tube

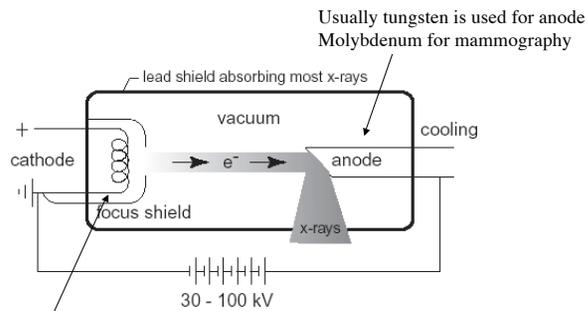


(a)
Tungsten filament heated to about 2200 C leading to thermionic emission of electrons.

TT Liu, BE280A, UCSD Fall 2006

Suetens 2002


X-Ray Production

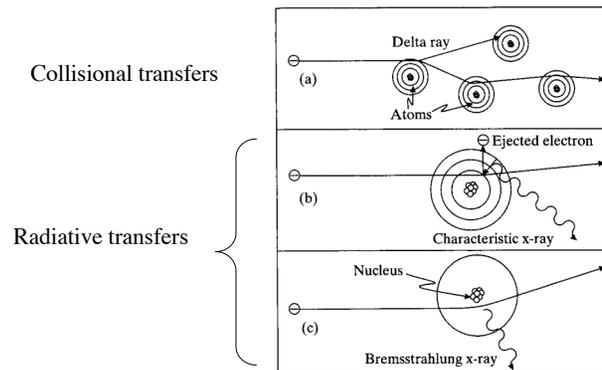

Prince and Links 2005

TT Liu, BE280A, UCSD Fall 2006

X-Ray Spectrum

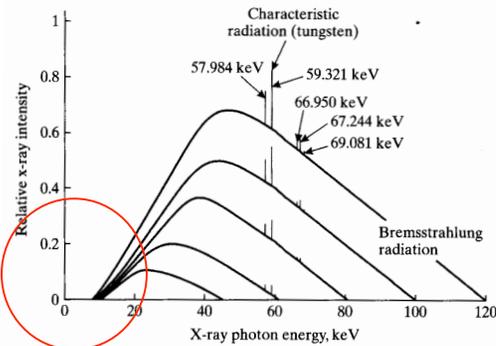

Lower energy photons are absorbed by anode, tube, and other filters

TT Liu, BE280A, UCSD Fall 2006


Prince and Links 2005

Interaction with Matter

Typical energy range for diagnostic x-rays is below 200 keV.

The two most important types of interaction are photoelectric absorption and Compton scattering.


Photoelectric effect dominates at low x-ray energies and high atomic numbers.

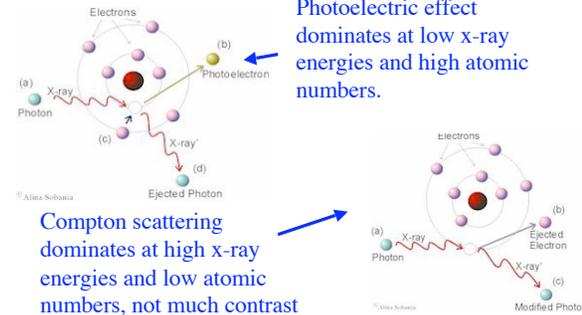

TT Liu, BE280A, UCSD Fall 2006


<http://www.eec.ntu.ac.uk/research/vision/asobania>

Interaction with Matter

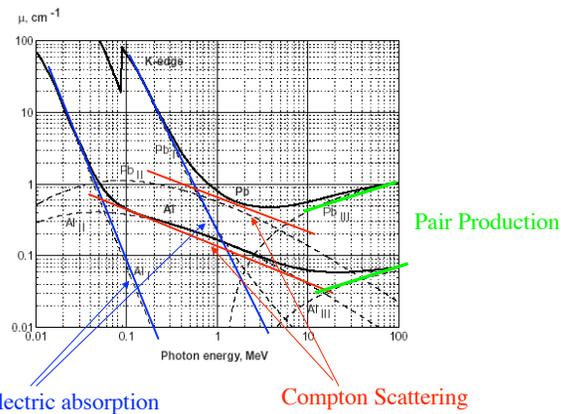

TT Liu, BE280A, UCSD Fall 2006

Attenuation

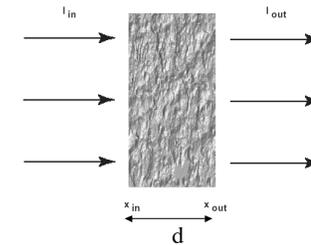


For single-energy x-rays passing through a homogenous object:

$$I_{out} = I_{in} \exp(-\mu d)$$

Linear attenuation coefficient

TT Liu, BE280A, UCSD Fall 2006

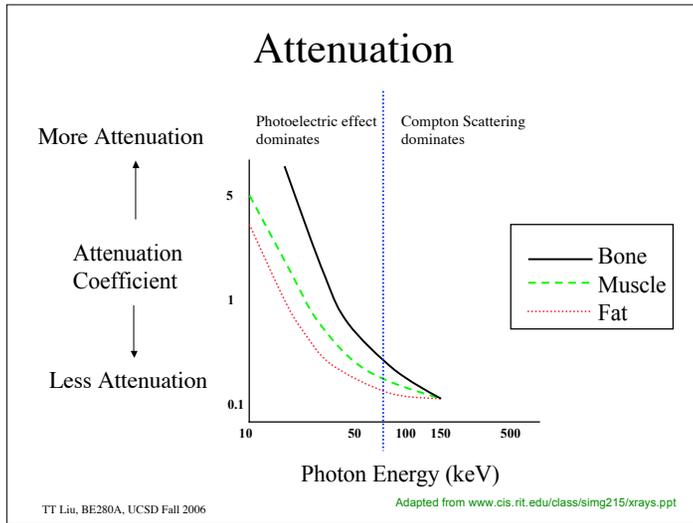

Half Value Layer

X-ray energy (keV)	HVL, muscle (cm)	HVL, Bone (cm)
30	1.8	0.4
50	3.0	1.2
100	3.9	2.3
150	4.5	2.8

In chest radiography, about 90% of x-rays are absorbed by body. Average energy from a tungsten source is 68 keV. However, many lower energy beams are absorbed by tissue, so average energy is higher. This is referred to as beam-hardening, and reduces the contrast.

Values from Webb 2003

TT Liu, BE280A, UCSD Fall 2006

Attenuation

For an inhomogeneous object:


$$I_{out} = I_{in} \exp\left(-\int_{x_{in}}^{x_{out}} \mu(x) dx\right)$$

Integrating over energies

$$I_{out} = \int_0^{\infty} \sigma(E) \exp\left(-\int_{x_{in}}^{x_{out}} \mu(E, x) dx\right) dE$$


Intensity distribution of beam

TT Liu, BE280A, UCSD Fall 2006

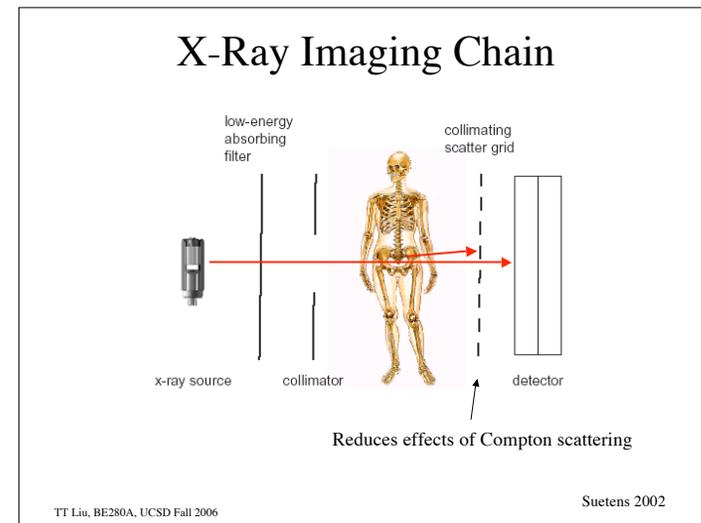

X-ray film

Emulsion with silver halide crystals
Each layer
~ 10 μm




Flexible base
~ 150 μm

Silver halide crystals absorb optical energy. After development, crystals that have absorbed enough energy are converted to metallic silver and look dark on the screen. Thus, parts in the object that attenuate the x-rays will look brighter.

TT Liu, BE280A, UCSD Fall 2006



Intensifying Screen

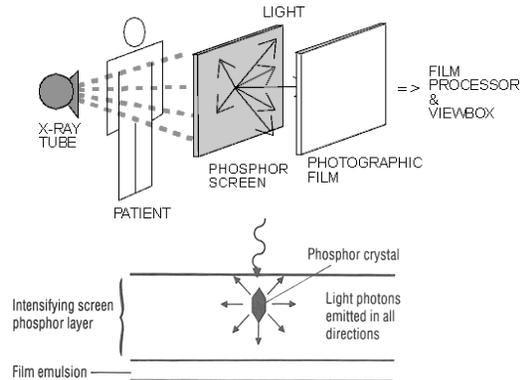

http://learntech.uwv.ac.uk/radiography/RScience/imaging_principles_d/diagram11.htm
<http://www.sunnybrook.utoronto.ca:8080/~selenium/xray.html#Film>

TT Liu, BE280A, UCSD Fall 2006

X-Ray Examples

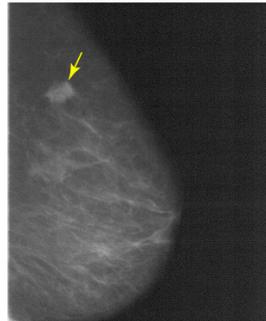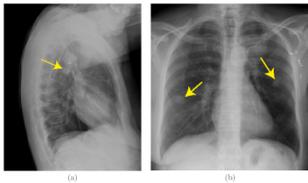


TT Liu, BE280A, UCSD Fall 2006

Suetens 2002

X-Ray w/ Contrast Agents



Angiogram using an iodine-based contrast agent.
K-edge of iodine is 33.2 keV




Barium Sulfate
K-edge of Barium is 37.4 keV

TT Liu, BE280A, UCSD Fall 2006

Suetens 2002


Contrast

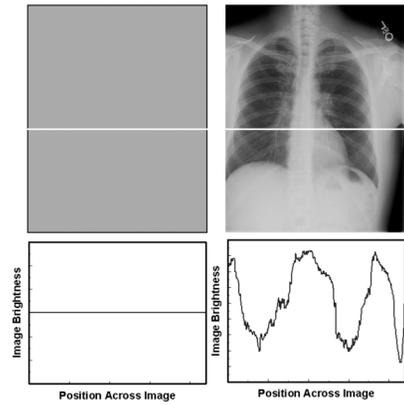


TT Liu, BE280A, UCSD Fall 2006

Bushberg et al 2001

Contrast

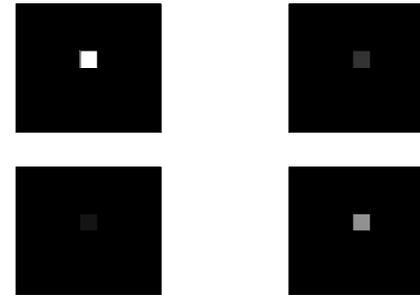

TT Liu, BE280A, UCSD Fall 2006

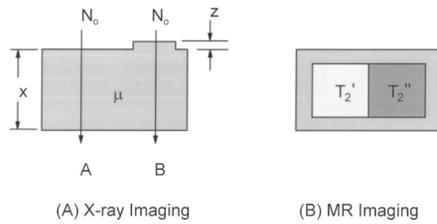

Bushberg et al 2001

$$A = N_0 \exp(-\mu x)$$

$$B = N_0 \exp(-\mu(x+z))$$

Subject Contrast

$$C_s = \frac{A-B}{A}$$

$$= \frac{N_0 \exp(-\mu x) - N_0 \exp(-\mu(x+z))}{N_0 \exp(-\mu x)}$$

$$= 1 - \exp(-\mu z)$$

TT Liu, BE280A, UCSD Fall 2006